

cobas[®] PCR Media Dual Swab Sample Kit

For in vitro diagnostic use

cobas[®] PCR Media Dual Swab Sample Kit

P/N: 07958021190

Table of contents

Intended use				
Reagents and materials4				
cobas [®] PCR Media Dual Swab Sample Kit4				
Precautions and handling requirements5				
Warnings and precautions5				
Reagent handling5				
Good laboratory practice5				
Specimen collection				
Endocervical swab specimen collection				
Specimen transport and storage7				
Vaginal swab specimen- clinician collection				
Specimen transport and storage8				
Vaginal swab specimen- self-collection in a clinical setting9				
Specimen transport and storage10				
Rectal swab specimen collection11				
Throat swab specimen collection13				
Additional information15				
Symbols15				
Manufacturer and distributors16				
Trademarks and patents16				
Copyright16				
References				
Document revision17				

Intended use

The cobas® PCR Media Dual Swab Sample Kit is used to collect and transport human specimens. The cobas® PCR Media serves as a nucleic acid stabilizing transport and storage medium for human specimens.

Note: This collection kit has been validated for use with cobas® CT/NG Tests.

Refer to the assay-specific Instructions for Use for particular specimen claims.

Reagents and materials

cobas[®] PCR Media Dual Swab Sample Kit

All unopened kits shall be stored as recommended in Table 1.

 Table 1
 cobas[®] PCR Media Dual Swab Sample Kit

cobas [®] PCR Media Dual Swab Sample Kit Store at 15-30°C 100 Packets (P/N 07958021190)					
cobas [®] PCR Media	≤ 40% (w/w) Guanidine hydrochloride Tris-HCl buffer	1 x 4.3 mL			
			Warning H302: Harmful if swallowed.		
			H315: Causes skin irritation.		
			H319: Causes serious eye irritation.		
			P264: Wash skin thoroughly after handling.		
			P270: Do not eat, drink or smoke when using this product.		
			P280: Wear protective gloves/ eye protection/ face protection.		
			P301 + P312 + P330: IF SWALLOWED: Call a POISON CENTER or doctor/ physician if you feel unwell. Rinse mouth.		
			P337 + P313: If eye irritation persists: Get medical advice/ attention.		
			P501: Dispose of contents/ container to an approved waste disposal plant.		
Dual Swab	1 woven swab (polyester bud)	2 $\stackrel{\circ}{_{ m 2}}$ swabs	Not applicable		

*Product safety labeling primarily follows EU GHS guidance

Swab)

1 flocked swab (polyester Hydra Flocked

Envelope

Precautions and handling requirements

Warnings and precautions

cobas[®] PCR Media contains guanidine hydrochloride. Do not allow direct contact between guanidine hydrochloride and sodium hypochlorite (bleach) or other highly reactive reagents such as acids and bases. These mixtures can release a noxious gas.

- For *in vitro* diagnostic use only.
- Carefully follow the instructions, as shown below.
- Avoid contact of the **cobas**[®] PCR Media with the skin, eyes or mucous membranes. If contact does occur, immediately wash with large amounts of water.
- If the collected specimen contains excess blood (specimen has a red or brown color), it should be discarded and not used for testing.
- Specimens should be handled as if infectious using safe laboratory procedures such as those outlined in Biosafety in Microbiological and Biomedical Laboratories¹ and in the CLSI Document M29-A4.²
- Safety Data Sheets (SDS) are available on request from your local Roche representative.

Reagent handling

- If cobas[®] PCR Media is spilled, FIRST clean with a suitable laboratory detergent and water, and then with 0.5% sodium hypochlorite.
- Dispose of unused reagents, waste and specimens in accordance with all applicable regulations.
- Do not use a kit after its expiration date.
- Ensure that the cap is tightened when closing the **cobas**[®] PCR Media Tube.
- Do not pre-wet swab in cobas® PCR Media before collection.


Good laboratory practice


- Always follow Good Laboratory Practices/Good Clinical Practices (GLP/GCP).
- Wear protective disposable gloves, coats, and eye protection when handling specimens and kit reagents. Wash hands thoroughly after handling specimens and kit reagents.

Specimen collection

Endocervical swab specimen collection

WARNING: DO NOT PRE-WET SWAB IN cobas® PCR MEDIA BEFORE COLLECTION!

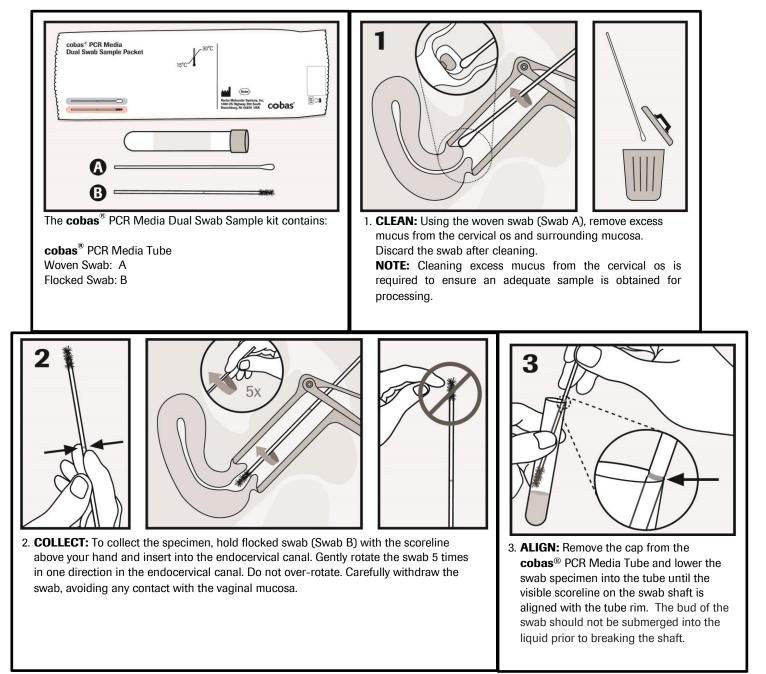


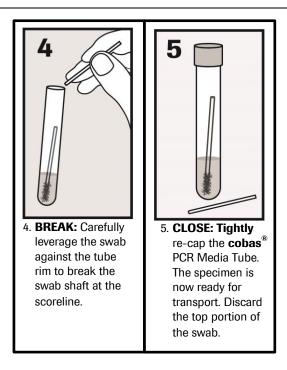


- Following specimen collection, transport and store the **cobas**® PCR Media Tube containing the collection swab at 2°C to 30°C.
- Consult the test-specific Instructions for Use for collected specimen stability claims.
- Transportation of collected specimens must comply with all applicable regulations for the transport of etiologic agents.³

Vaginal swab specimen- clinician collection


WARNING: DO NOT PRE-WET SWAB IN cobas[®] PCR MEDIA BEFORE COLLECTION!

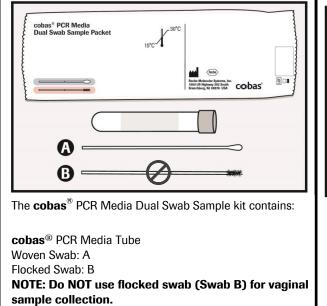

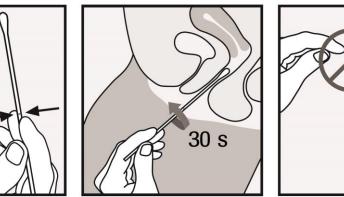

1. **COLLECT :** In one hand, hold the woven swab (Swab A) with the scoreline above your hand and insert the swab about 5 cm (2 inches) into the vaginal opening. Gently turn the swab for about 30 seconds while rubbing the swab against the walls of the vagina.


Withdraw the swab carefully. Do not let the swab touch any surface before placing it into the collection tube.

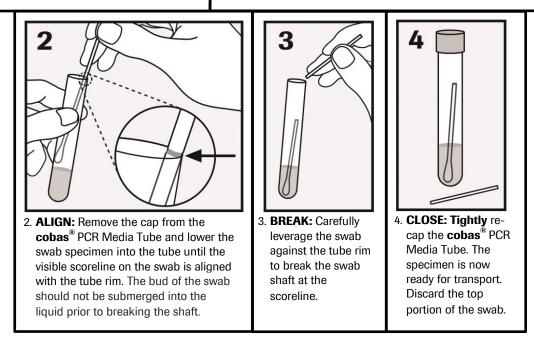


- Following specimen collection, transport and store the **cobas**[®] PCR Media Tube containing the collection swab at 2°C to 30°C.
- Consult the test-specific Instructions for Use for collected specimen stability claims.
- Transportation of collected specimens must comply with all applicable regulations for the transport of etiologic agents.³

Vaginal swab specimen- self-collection in a clinical setting

WARNING: DO NOT PRE-WET SWAB IN cobas® PCR MEDIA BEFORE COLLECTION!

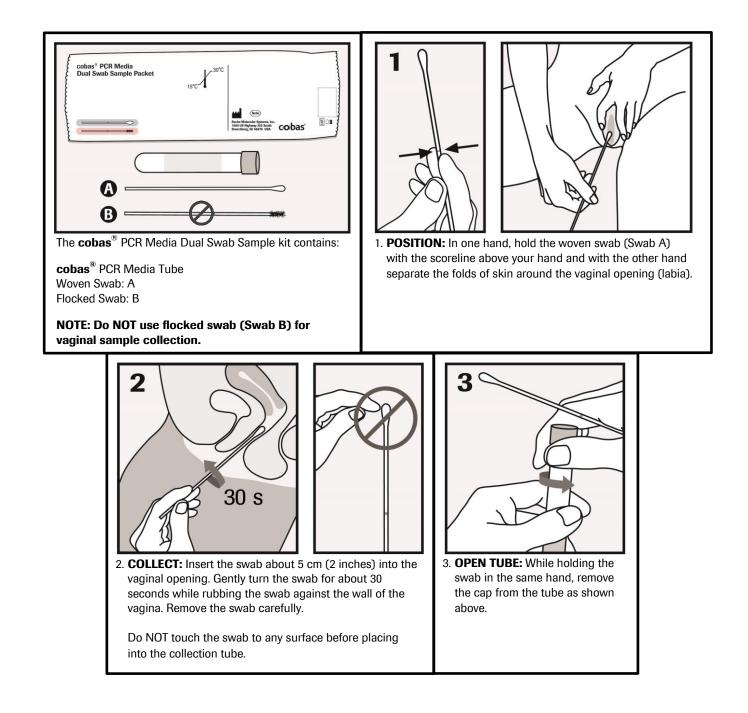


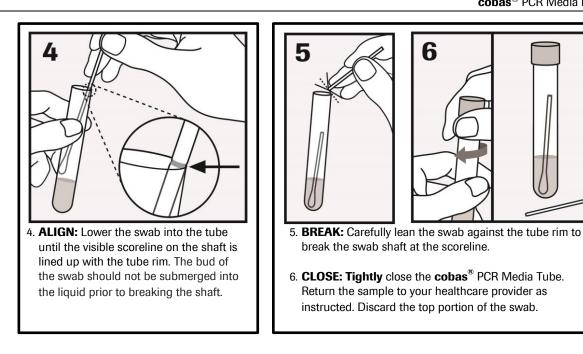

- Following specimen collection, transport and store the **cobas**[®] PCR Media Tube containing the collection swab at 2°C to 30°C.
- Consult the test-specific Instructions for Use for collected specimen stability claims.
- Transportation of collected specimens must comply with all applicable regulations for the transport of etiologic agents.³


Rectal swab specimen collection

WARNING: DO NOT PRE-WET SWAB IN cobas® PCR MEDIA BEFORE COLLECTION!

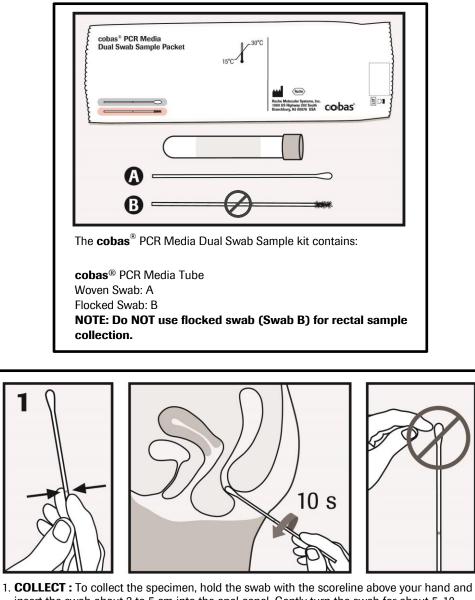

insert the swab about 3 to 5 cm into the anal canal. Gently turn the swab for about 5-10 seconds while running the swab against the walls of the rectum. If the swab is grossly contaminated with feces, discard and repeat the collection.


Withdraw the swab carefully. Do not let the swab touch any surface before placing it into the collection tube.

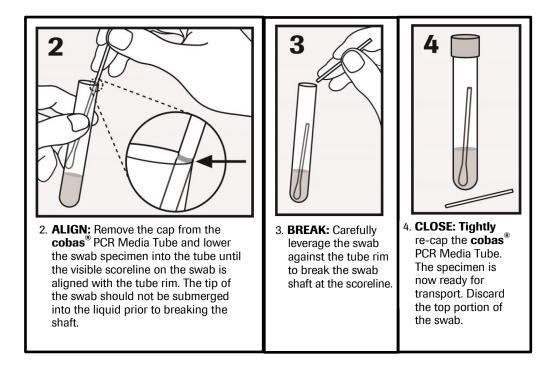



- Following specimen collection, transport and store the **cobas**[®] PCR Media Tube containing the collection swab at 2°C to 30°C.
- Consult the test-specific Instructions for Use for collected specimen stability claims.
- Transportation of collected specimens must comply with all applicable regulations for the transport of etiologic agents.³

Throat swab specimen collection

WARNING: DO NOT PRE-WET SWAB IN cobas® PCR MEDIA BEFORE COLLECTION!

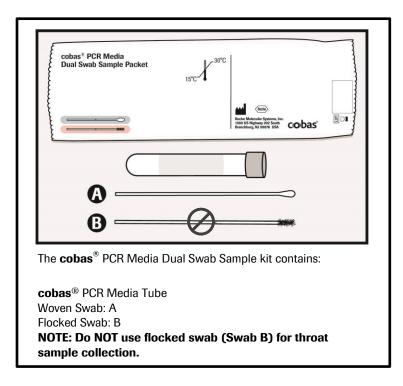

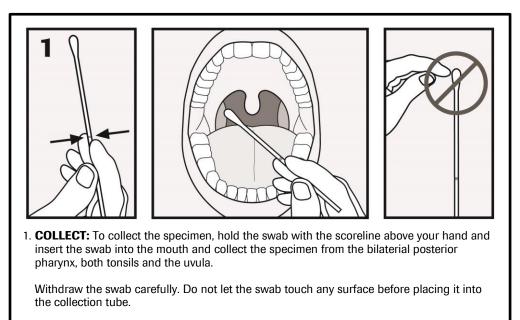

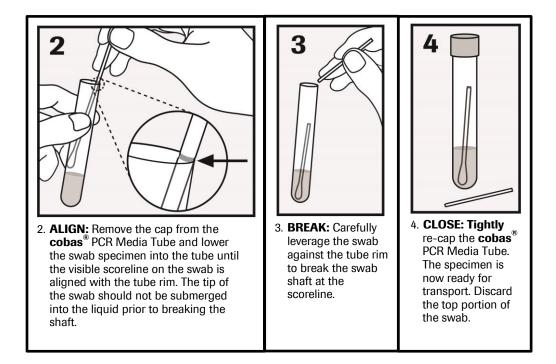


- Following specimen collection, transport and store the **cobas**® PCR Media Tube containing the collection swab at 2°C to 30°C.
- Consult the test-specific Instructions for Use for collected specimen stability claims.
- Transportation of collected specimens must comply with all applicable regulations for the transport of etiologic agents.³

Additional information

Symbols

The following symbols are used in labeling for Roche PCR diagnostic products.

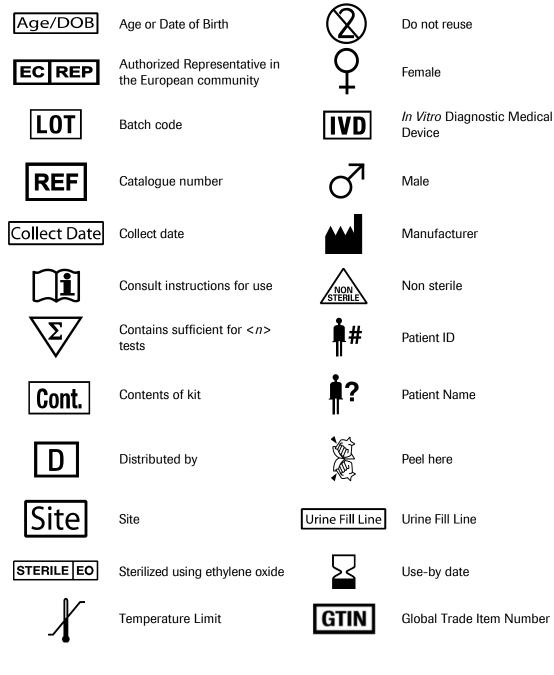

This product fulfills the requirements of the European Directive 98/79 EC for *in vitro* diagnostic medical devices.

US Customer Technical Support 1-800-526-1247

CE

Manufacturer and distributors

Manufactured for:



Roche Molecular Systems, Inc.

1080 US Highway 202 South Branchburg, NJ 08876 USA www.roche.com



Roche Diagnostics 201, boulevard Armand-Frappier H7V 4A2 Laval, Québec, Canada (For Technical Assistance call: Pour toute assistance technique, appeler le: 1-877-273-3433)

Distributore in Italia: Roche Diagnostics S.p.A Viale G. B. Stucchi 110 20052 Monza, Milano, Italy

Roche Diagnostics GmbH Sandhofer Strasse 116 68305 Mannheim, Germany

Roche Diagnostics (Schweiz) AG Industriestrasse 7 6343 Rotkreuz, Switzerland Roche Diagnostics, SL Avda. Generalitat, 171-173 E-08174 Sant Cugat del Vallès Barcelona, Spain

Distribuidor em Portugal: Roche Sistemas de Diagnósticos Lda. Estrada Nacional, 249-1 2720-413 Amadora, Portugal

Roche Diagnostics 2, Avenue du Vercors 38240 Meylan, France

Roche Diagnostica Brasil Ltda. Av. Engenheiro Billings, 1729 Jaguaré, Building 10 05321-010 São Paulo, SP Brazil

Trademarks and patents

See http://www.roche-diagnostics.us/patents

Copyright

©2017 Roche Molecular Systems, Inc.



Roche Diagnostics GmbH Sandhofer Str. 116 68305 Mannheim Germany





References

- 1. Center for Disease Control and Prevention. Biosafety in Microbiological and Biomedical Laboratories, 5th ed. U.S. Department of Health and Human Services, Public Health Service, Centers for Disease Control and Prevention, National Institutes of Health HHS Publication No. (CDC) 21-1112, revised December 2009.
- 2. Clinical and Laboratory Standards Institute (CLSI). Protection of laboratory workers from occupationally acquired infections. Approved Guideline-Fourth Edition. CLSI Document M29-A4:Wayne, PA;CLSI, 2014.
- 3. International Air Transport Association. Dangerous Goods Regulations, 52nd Edition. 2011.

Document revision

Document Revision Information			
Doc Rev. 1.0 11/2016	First Publishing.		
Doc Rev. 2.0 05/2017	 Added statement "Refer to the assav-specific Instructions for Use for particular specimen claims" and removed reference to cobas[®] CT/NG v2.0 Test in the Intended use section. Changed "gynecological specimens" to "human specimens" in the Intended use section. Added collection instructions for oropharyngeal swab specimens and anorectal swab specimens. Please contact your local Roche Representative if you have any questions. 		